

Pipette Management Solutions by A&D



For quick checking of pipette airtightness...
Leak Tester: AD-1690

*To protect research results from
the threat of nonconformities*



For verification of pipette accuracy and precision...
Pipette Accuracy Testers:
BM Series + BM-014, etc.

For easy implementation of daily and periodic pipette checks...
Pipette Professional: AD-1695



A&D ...Clearly a Better Value
A&D Company, Limited
<http://www.aandd.jp>

*What If You Were Told to Create a Pipette Management SOP^{*1} Within Three Weeks?*

*1 Standard Operating Procedure

Today, what with GLP and ISO, researchers are in increasing need of sustainable ways to verify the quality and performance of their pipettes in-house. The problem is, however, that many of them would be at a loss as to what exactly they should put into actual practice. Wouldn't you be too?

Not to worry, though. A&D provides the following powerful solutions that you can use to introduce a simple, viable SOP for pipette management.

For Daily Checks

Leak Tester AD-1690



Pipette failures typically occur due to degraded parts in the lower section of the pipette like the o-ring, piston, and tip holder compromising the pipette's airtightness. By depressurizing (to -20 kPa) inside the pipette, the AD-1690 can determine whether an air leak exists in a matter of seconds, allowing you to quickly sort out troubled pipettes.

A&D suggests that for everyday inspection, this leak test along with some quick appearance and function checkups will suffice for most users.

Advantages

- ✓ Takes only seconds to tell whether the pipette has a leak
- ✓ Changes pressure by evacuating air instead of injecting it^{*2}, so that no dust enters the pipette being tested
- ✓ Easily replaceable air filter, which protects the AD-1690 from dust when it intakes air
- ✓ Equipped with an RS-232C interface to output test results to an external device such as the AD-1695 Pipette Professional (see later pages)
- ✓ Four attachments and one adapter tube provided to fit various tip sizes and shapes



Air filter unit

*2 A pressurization method is available upon request.

For Periodic Checks

Pipette Accuracy Testers



AD-4212B-PT



AD-4212A-PT



FX-300i-PT

In addition to the daily check, you are advised to inspect the pipettes' actual performance from time to time. For that purpose, A&D's pipette accuracy testers are useful. The test procedure follows the gravimetric method^{*3} and allows compliance with ISO8655.

*3 Obtains the pipette volume based on the mass of purified water dispensed from the pipette

Advantages

- ✓ Automatic mass-to-volume conversions and judgments for accuracy and repeatability using the special “WinCT-Pipette” software
- ✓ Judgments by your preferred criteria – manufacturer specifications, ISO8655, or your own
- ✓ Outputs the test results in an A4 or letter-size report format for documentation requirements
- ✓ A liquid thermometer, evaporation trap, and calibration weight with a pair of tweezers included as standard
- ✓ Comes packed neatly in a handy carrying case for use in multiple places*⁴*⁵


*⁴ For the AD-4212B-PT, AD-4212A-PT, and FX-300i-PT only

*⁵ Not advisable when using the 0.001 mg range of the AD-4212B-PT

Evaporation Trap*

The evaporation trap maintains a high humidity inside the device and thereby minimizes the evaporation of the test liquid that causes measurement errors. It is no longer necessary to increase the humidity of an entire room.

★ Patent pending

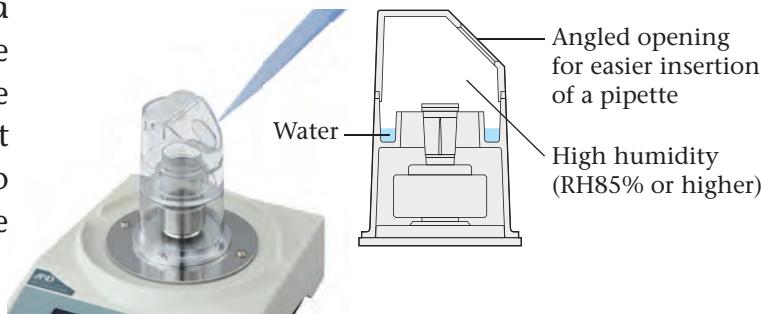

WinCT-Pipette

Main screen

No.	(µL)	(mg)
1	49.72	49.55
2	49.74	49.57
3	49.80	49.63
4	49.76	49.71
5	49.74	49.57
6	49.72	49.51
7	49.76	49.61
8	49.80	49.63
9	49.80	49.71
10	49.80	49.63

Test report

Pipette	Mean (µL)	Z Factor	Status
AD-4212B-101	49.752	1.0035	Pass
AD-4212A-101	49.752	1.0035	Pass
FX-300i-101	49.752	1.0035	Pass
AD-4212B-102	49.752	1.0035	Pass

WinCT-Pipette automatically determines the Z (conversion) factor based on the entered test liquid (i.e. purified water) temperature and barometric pressure, which is then used to calculate volumes from the mass values transmitted from the balance.

Information for each pipette (including manufacturer, model, and test conditions and specifications) can be saved and retrieved for later testing.*⁶

*⁶ It is recommended that the database be backed up on a regular basis.

Also available...

Micro Analytical Balances ***BM Series + BM-014***

The BM-014 can be used with any model of the BM series (both 5 mL and 30 mL cups are provided). This setup is ideal if you also want to use the balance for purposes other than pipette accuracy testing as an ordinary analytical balance.



Recommended Models in Accordance With ISO8655

Pipette Nominal Volume ^{◆1}	ISO8655 Requirements (Gravimetric Method)				Balance Readability	Recommended Models			
	Maximum Permissible Error		Accuracy (Systematic Error)	Repeatability (Random Error)					
	%	±µL		mg					
(µL)	±%	±µL	%	µL	mg				
1	5.0	0.05	5	0.05	0.001	BM-20/22 + BM-014		(◆2)	
2	4.0	0.08	2	0.04					
5	2.5	0.125	1.5	0.075					
10	1.2	0.12	0.8	0.08					
20	1.0	0.2	0.5	0.1	0.01	BM-252 + BM-014	AD-4212B-PT		
50	1.0	0.5	0.4	0.2					
100	0.8	0.8	0.3	0.3					
200	0.8	1.6	0.3	0.6					
500	0.8	4.0	0.3	1.5	0.1	BM-200/300/500 + BM-014 or AD-4212A-PT			
1000	0.8	8.0	0.3	3.0					
2000	0.8	16	0.3	6.0					
5000	0.8	40	0.3	15.0					
10000	0.6	60	0.3	30.0					
Daily inspection, simplified verification				1 ^{◆3}		FX-300i-PT			

◆1 The maximum volume selectable for variable volume pipettes

◆2 Please select the BM-20/22 + BM-014 if you will mainly use the 0.001 mg range, as it will provide much greater stability.

◆3 The minimum weighing value, 1 mg, approximately corresponds to 1 µL. If a pipette volume is 1000 µL, a test can be performed with a resolution of 0.1%. If 200 µL, 0.5%.

Note) Make sure that the measurement environment is free from vibration, drafts, rapid temperature/humidity changes, etc.

Single Channel Electronic Pipettes ***MPA Series***



Supposing that some of your pipettes have been found inaccurate by your periodic check, what should you do? If you use the MPA series, it is easy to correct deviations by yourself. All you have to do is simply input the actual dispensed volume measured by a pipette accuracy tester into the pipette.*

★ Patent pending

... Still not comfortable enough with what you should do? Then how about getting some professional help?

For “Guided” Checks

Pipette Professional AD-1695



Stop dwelling on how to put the said tasks and tools in order by yourself. Leave everything to the AD-1695. All you have to do is follow the displayed instructions and touch the screen to enter necessary information, commands, selections, etc., so you can perform daily and periodic checks in ways already laid out by A&D for you.

Daily check (basic check) function

01/01/2015 21:21 A&D / Sample /SN: 12345678

Daily check (1/2)

Exterior appearance	Dirt, stains	Met <input checked="" type="checkbox"/>	Not met <input type="checkbox"/>
	Scratches, rust, damage to parts	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Moving parts	Operation button	<input checked="" type="checkbox"/>	<input type="checkbox"/>
	Volume meter	<input type="checkbox"/>	<input checked="" type="checkbox"/>
	Ejector	<input checked="" type="checkbox"/>	<input type="checkbox"/>

Pipette Select >> Home

For daily checks, you are simply asked to determine whether the condition is “met” or “not met” for each check item. The check items include those which A&D recommends as the most basic ones to confirm that the pipette meets proper conditions for use.

01/01/2015 21:21 A&D / Sample /SN: 12345678

Daily check (2/2)

Leak	Use an AD-1690 (leak tester): AD-1690 COM 1 Result -19.9kPa Start PASS	Met <input checked="" type="checkbox"/>	Not met <input type="checkbox"/>
	When water is aspirated and left inside, no drops form on the end of the pipette.		
	When water is aspirated and the pipette tip is dipped into the liquid container, the liquid level inside the tip does not drop.		

Pipette Select Mini printer COM 3 Print USB PDF << Home

To perform an air leak test, you can choose (and are encouraged) to connect and use the AD-1690 Leak Tester, which the AD-1695 can control and capture the result from to make the met/not met judgment promptly and automatically.*7

*7 Testing without the AD-1690 also possible (albeit time-consuming and often difficult to judge)

Periodic check (volume test) function



The AD-1695 enables you to easily test for pipette volume accuracy and repeatability by connecting it to one of A&D's balances^{*8}. All the key functions provided by WinCT-Pipette are also available on the AD-1695, so that you can complete both the basic check and volume test one after another without using a PC.

*8 Either the pipette accuracy testers or the BM series with BM-014 are strongly recommended, as they come with an evaporation trap and other useful accessories.

Reporting results

The daily and periodic check results can be output to a USB flash drive in PDF report formats. A reference number, location name, and operator name can be added as necessary.

It is also possible to output the results directly to a standard mini printer.*⁹

*9 In simplified formats


Daily Pipette Check Report		
1. Pipette information		
Manufacturer	A&D	
Model	Sample	
Serial No.	12345678	
Machine value	1200.0 (uL)	
2. Confirmation of exterior appearance		
The pipette unit is clean.....	Met	
There are no scratches, dent, rust or damaged parts on the pipette.....	Not met	
3. Confirmation of moving parts		
The operation lever works smoothly.....	Met	
The volume lever works smoothly.....	Not met	
The tip ejection lever works smoothly.....	Met	
4. Confirmation of leak		
Airtightness is guaranteed.....	Met	
Measurement results with AD-1695 (last meter), -19.9kPa T100121		
5. Test information		
Reference number	0001	
Date of measurement	2015/01/01	
Location of measurement	A&D	
Remarks		
Signature (Operator) TEST		
Signature (Manager)		

Daily check report (PDF)

Pipette periodic check report			
1. Pipette information			
Manufacturer	A&D		
Model	Sample		
Serial No.	12345678		
Machine value	1200.0 (uL)		
2. Environment			
Temperature	38.0 (°C)	38.0 (°C)	
Atmospheric pressure	1013.0 (hPa)	1013.0 (hPa)	
3. Basic functions			
Accuracy	Measuring point(1)	Measuring point(2)	
Absolute error	1.00 (uL)	0.99 (uL)	
Relative error	1.00 (%)	0.99 (%)	
Repeatability	0.50 (uL)	0.50 (uL)	
4. Measured value			
No.	Measuring point(1) (uL)	Measuring point(2) (uL)	Measuring point(3) (uL)
1	1198.0	1198.0	1198.0
2	1198.3	1198.0	1198.0
3	1198.3	1198.0	1198.0
4	1198.4	1198.0	1198.0
5	1198.3	1198.0	1198.0
6	1198.3	1198.0	1198.0
7	1198.0	1198.0	1198.0
8	1198.4	1198.0	1198.0
9	1198.3	1198.0	1198.0
10	1198.2	1198.0	1198.0
5. Results			
Number of measurements	10	10	
Absolute error	0.00 (uL)	0.00 (uL)	
Relative error	0.00 (%)	0.00 (%)	
Repeatability	0.00 (uL)	0.00 (uL)	
6. Test information			
Reference number	0001		
Date of measurement	2015/01/01		
Location of measurement	A&D		
Remarks			
Signature (Operator) TEST			
Signature (Manager)			

Periodic check report (PDF)

Pipette registration/selection and spec configuration

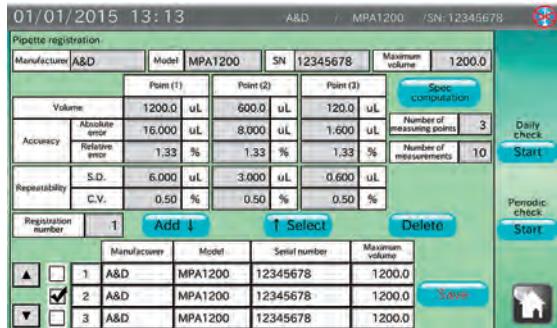

Up to 300 pipettes' information (manufacturer, model, serial number, and maximum volume) with volume test conditions and specifications can be registered in the AD-1695, which you can select and readout when conducting daily and periodic checks.

The registered information of the pipette checked will be automatically reflected in the output reports.

Glossary and quick manual

You can quickly call up the on-screen explanations of terms that are relevant or used on the AD-1695. There is also an on-screen instruction manual available for each of the daily check, periodic check, and pipette registration/selection operations. It will tell you what to do as you touch the number in the respective section.

With these functions, most of the time you are not required to look for or refer to any other resource for understanding and operating the AD-1695.

